

Operating Instructions



1 General Information.....	2
1.1 General Safety Notes.....	2
1.2 Intended Use.....	2
2 Transportation and Storage.....	2
3 Installation and Commissioning	2
3.1 Mechanical Installation.....	2
4 Operation.....	3
4.1 Zero-point correction	3
4.2 Maintenance / Service.....	3
5 Disassembly.....	4

1 General Information

This document contains necessary information for the proper installation and use of this device. In addition to this instruction, be sure to observe all statutory requirements, applicable standards, the additional technical specifications on the accompanying data sheet (see www.labom.com) as well as the specifications indicated on the type plate.

1.1 General Safety Notes

The installation, set up, service or disassembly of this device must only be done by trained, qualified personnel using suitable equipment and authorized to do so.



Warning

Media can escape if unsuitable devices are used or if the installation is not correct.

Danger of severe injury or damage

- Ensure that the device is suitable for the process and undamaged.

1.2 Intended Use

The device is intended to measure pressure of gases, vapors and liquids as specified in the data sheet.

2 Transportation and Storage

Store and transport the device only under clean and dry conditions preferably in the original packaging. Avoid exposure to shocks and excessive vibrations.

Permissible storage temperature: 0...70 °C

3 Installation and Commissioning

Ensure that the device is suitable for the intended application with respect to pressure range, overpressure limit, media compatibility, temperature range and process connection.

3.1 Mechanical Installation

Use gaskets, if required, that are suitable for the process connection and resistant to the media.

Before starting operation, check the process connection carefully for leaks under pressure.

Use new gaskets for each installation. We recommend the use of aluminium gaskets (A 27 x 32 as per DIN 7603), which you can order directly from us as an accessory.

Fit the pressure transmitter using four flange screws, as shown on the drilling diagram, and tighten them gradually crosswise. Max. tightening torque: 60 Nm (slightly oiled).

During installation of the device, attention has to be paid to the diaphragms not being damaged by the medium being measured. This is particularly important in the case of coagulating media that can have deforming influence on the diaphragms when they get cold.

Do not insulate the temperature coupler (tubular shank under the transmitter), as this would reduce its decoupling effect.




Figure 1: Drilling diagram

Vent the pressure gauge after installation using the vent valve (Figure 2).

The devices are supplied with a closed vent valve (CLOSED position). Moving the red lever to the OPEN position equalises the pressure level inside and outside the case (Figure 3).



Figure 2: Vent valve

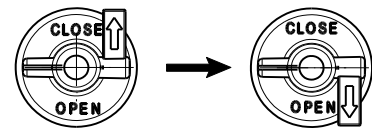


Figure 3: Move valve

4 Operation

During operation, take care that the device remains within its intended pressure and temperature ranges. No other monitoring is necessary.

Permissible media temperature: 10...350 °C

Permissible ambient temperature: 10...70 °C

4.1 Zero-point correction

Small measuring errors or deviations caused by difference in level between pressure gauge and point of measurement can be corrected on measuring devices with micro control position pointers. To do so turn the adjusting screw on the pointer hub (see figure 4).

Similarly, a displacement of the zero point caused by use and long service life can be corrected if necessary.



Figure 4: Zero-point correction

4.2 Maintenance / Service

When properly installed in accordance with applicable specifications, this device is maintenance-free. However, we recommend an annual recalibration of the device.

5 Disassembly

When measuring hot media, make sure that the device has cooled down prior to any dismounting or wear appropriate protective clothing to avoid burns.

Switch off the power supply to the device before disconnecting the electrical connections. Once this is done, the device may be mechanically removed.

Remove the four flange screws.

The pressure transmitter system may be pulled out only while the process medium is liquid (above melting point).

Use cylinder head screws (M12 x 55 as per DIN 912, A2-70) quality) for the two threaded holes, as shown on the drilling diagram, to push the device out of the process and ensure ease of removal. You can order these screws as an accessory.



Warning

Opening pressurized lines might cause severe injuries.

Danger of severe injuries or damage

- Relieve the process pressure before attempting to remove the device. Shut off the pressure supply for all feed lines to the device and relieve the pressure in them.



Warning

Hazardous deposits and residues might remain on opened process connections and removed devices.

Danger of injury

- After the device has been removed, seal off the measuring point and mark the open process connection accordingly. Consider a possible danger due to residues when handling the removed device.